Qualitative Analysis Report

Data Filename	TOX21_400063_TMS 1.D	**Sample Name**	NCGC Tox21_400063 from C05 SP109717
Position	53	**Instrument Name**	5975C_MR
User Name	Kirill	**Acq Method**	B1_28-0_2_520_mt384_sndv.M

User Chromatograms

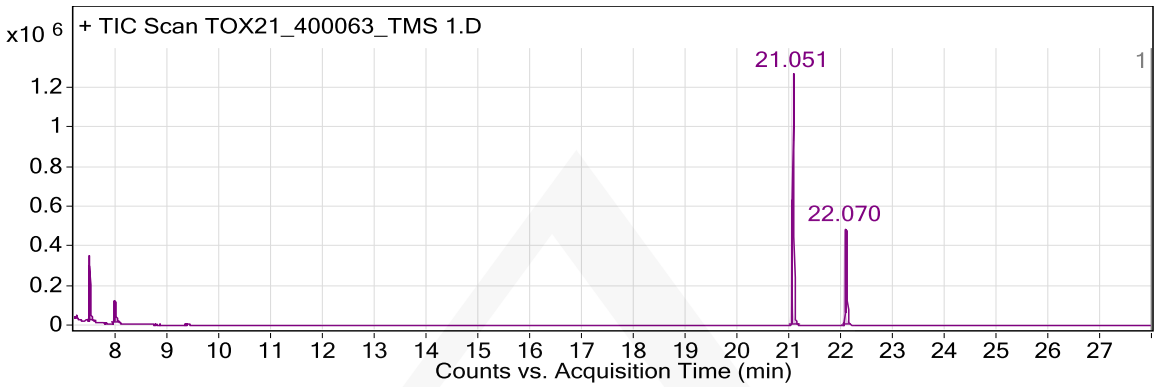

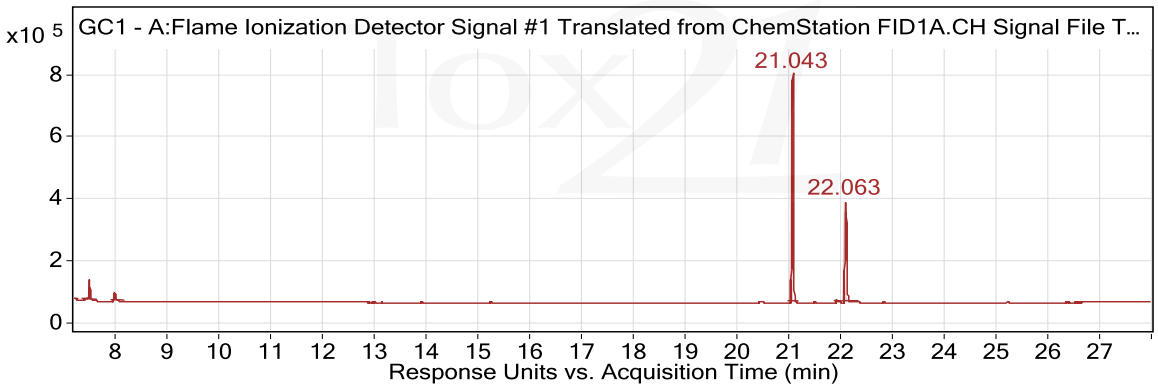

A MW Confirmed, Purity>90%

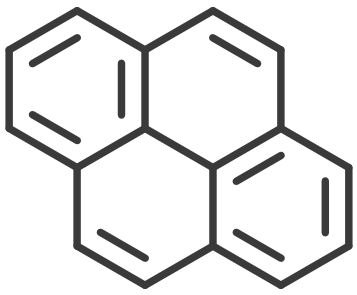

PubChem

User Spectra

Spectrum Source
Peak (1) in "+ TIC Scan"

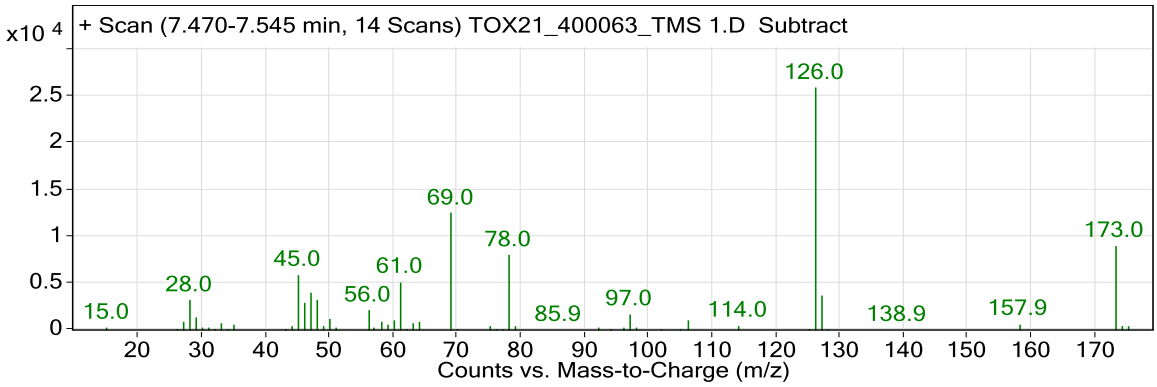

Spectrum Source
Peak (2) in "+ TIC Scan"

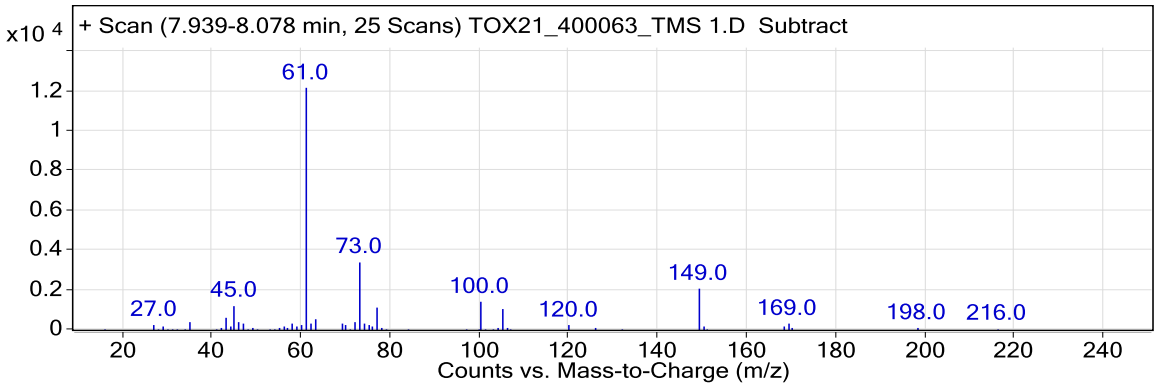

Spectrum Source
Peak (3) in "+ TIC Scan"

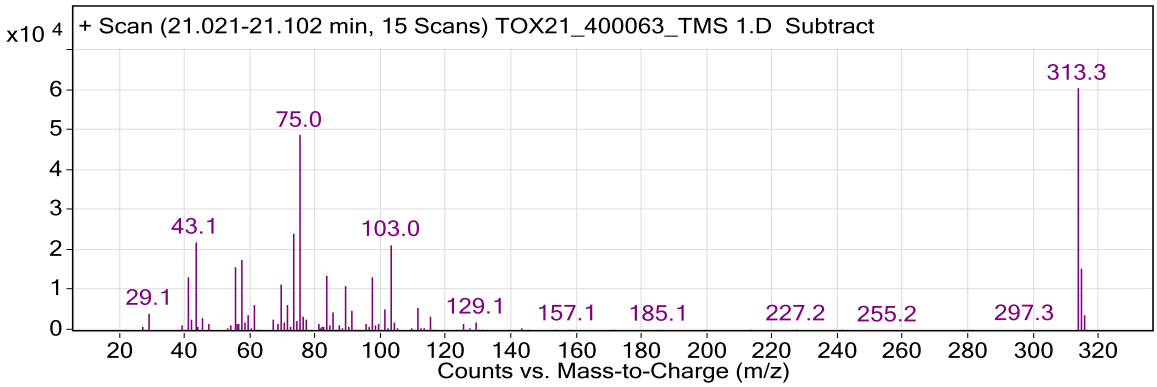

Spectrum Source
Peak (4) in "+ TIC Scan"

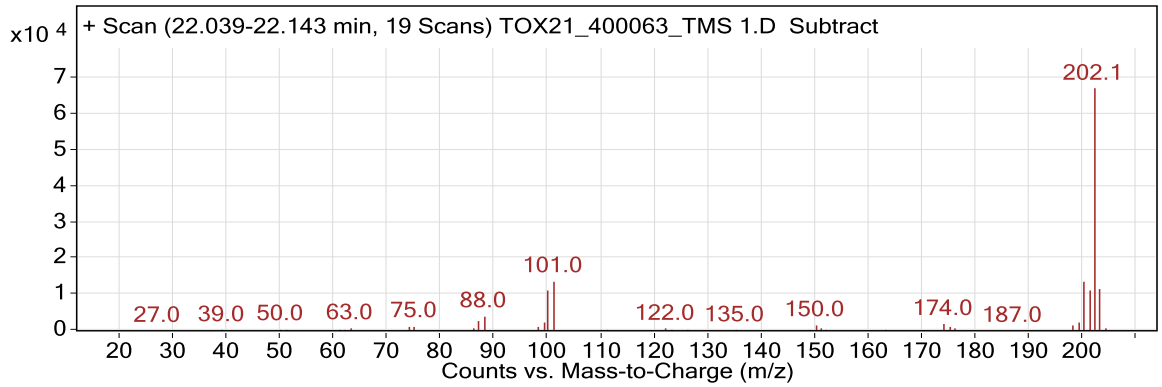

--- End Of Report ---

Qualitative Analysis Report

Data Filename	TOX21_400063_TMS 2.D	**Sample Name**	NCGC Tox21_400063 from E13 SP109722
Position	109	**Instrument Name**	5975C_MR
User Name	Kirill	**Acq Method**	C1_28-0_2_520_mt384_sndv.M

User Chromatograms

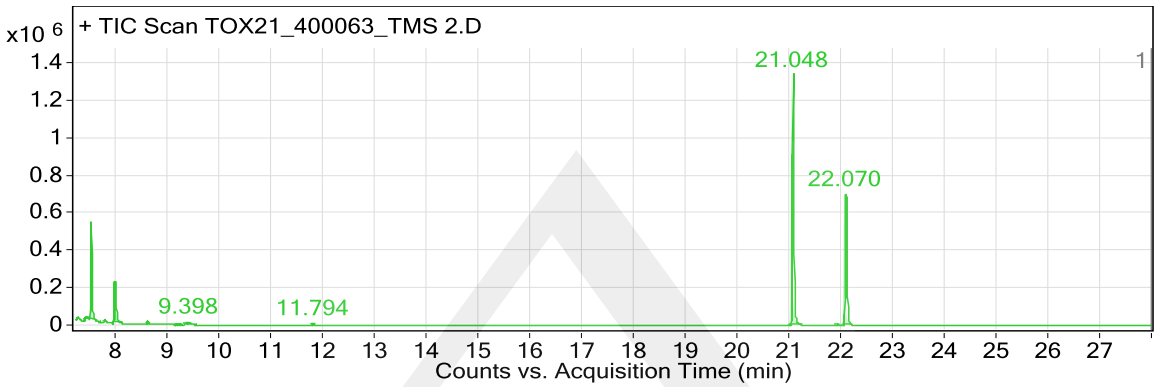

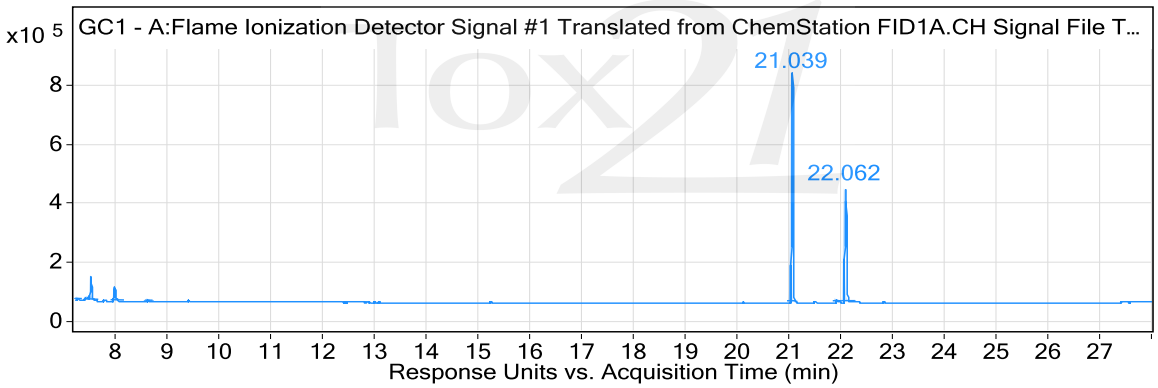

User Spectra

Spectrum Source
Peak (1) in "+ TIC Scan"

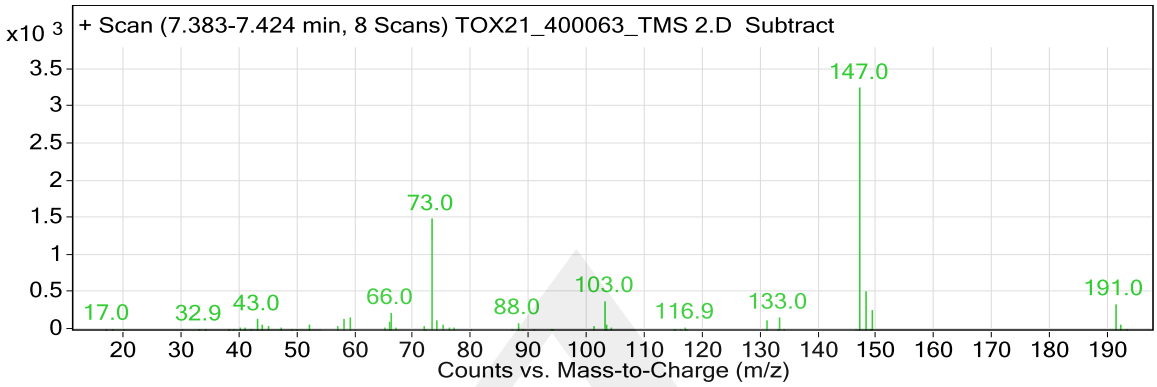

Spectrum Source
Peak (2) in "+ TIC Scan"

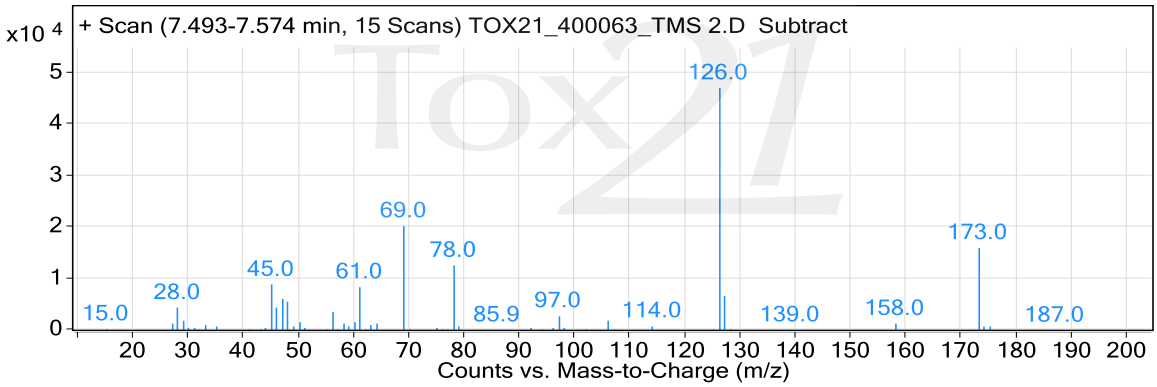

Spectrum Source
Peak (3) in "+ TIC Scan"

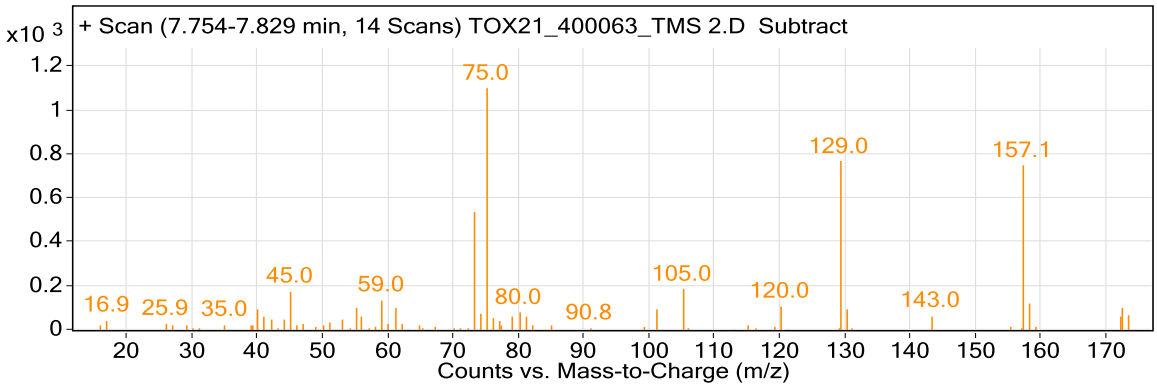

Spectrum Source
Peak (4) in "+ TIC Scan"

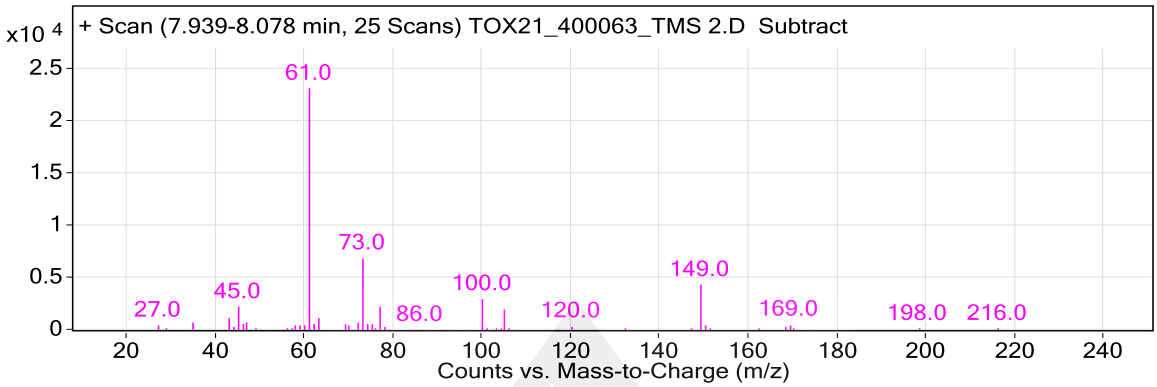

Spectrum Source
Peak (5) in "+ TIC Scan"

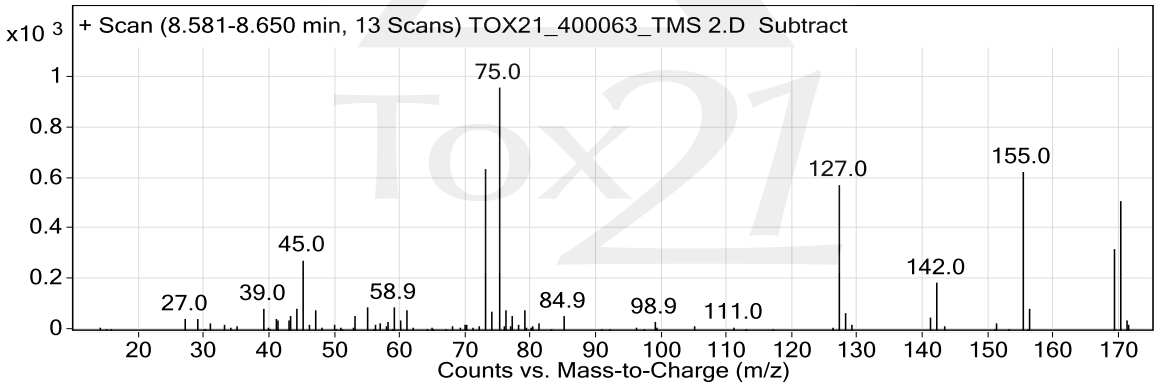

Spectrum Source
Peak (6) in "+ TIC Scan"

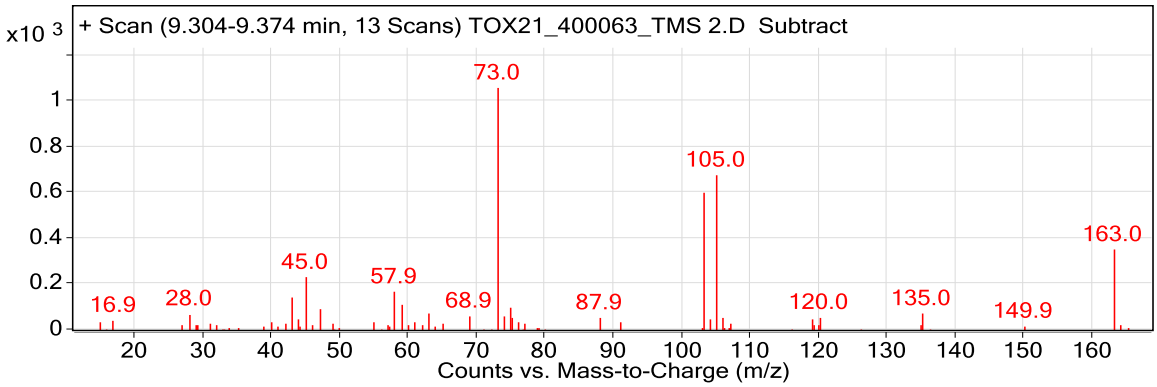

Spectrum Source
Peak (7) in "+ TIC Scan"

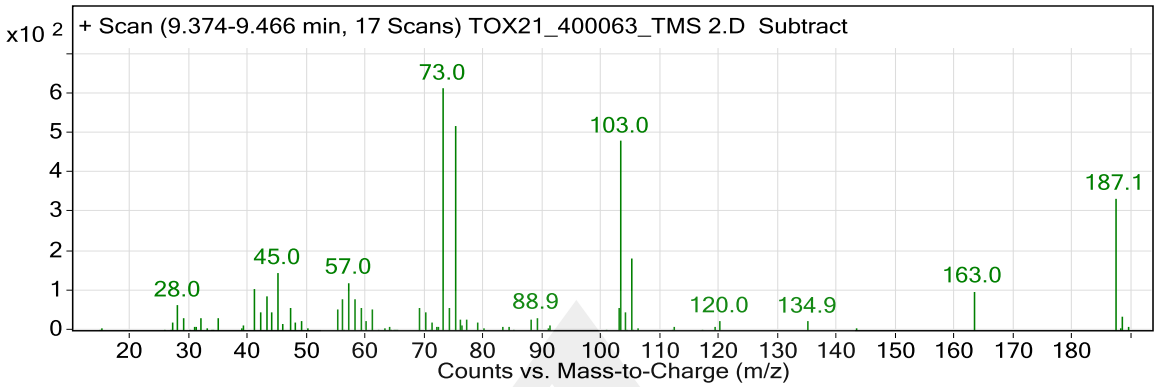

Spectrum Source
Peak (8) in "+ TIC Scan"

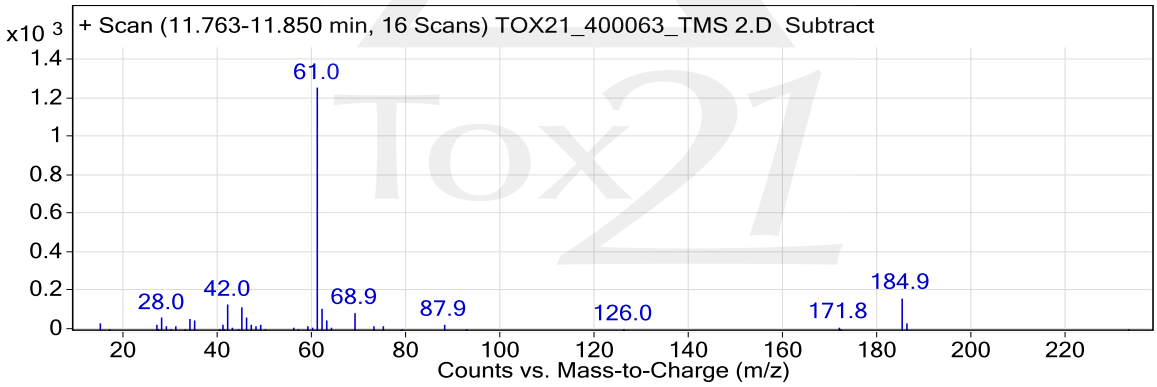

Spectrum Source
Peak (9) in "+ TIC Scan"

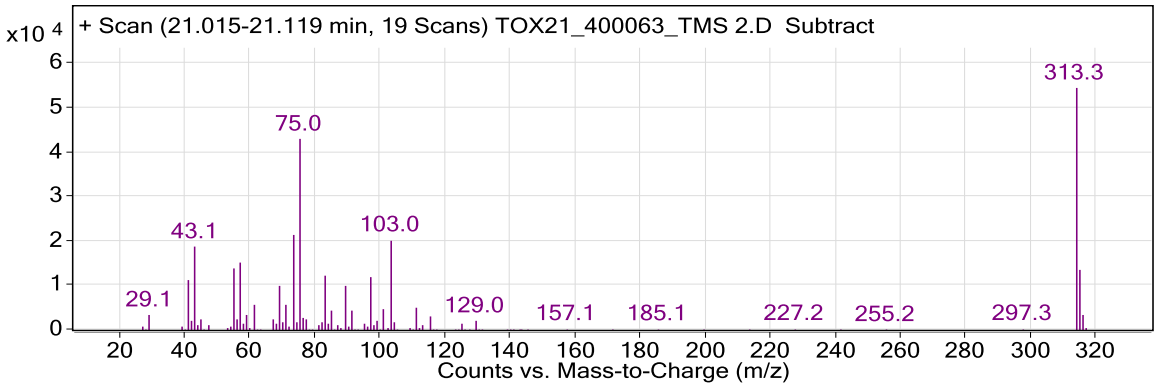

Spectrum Source
Peak (10) in "+ TIC Scan"

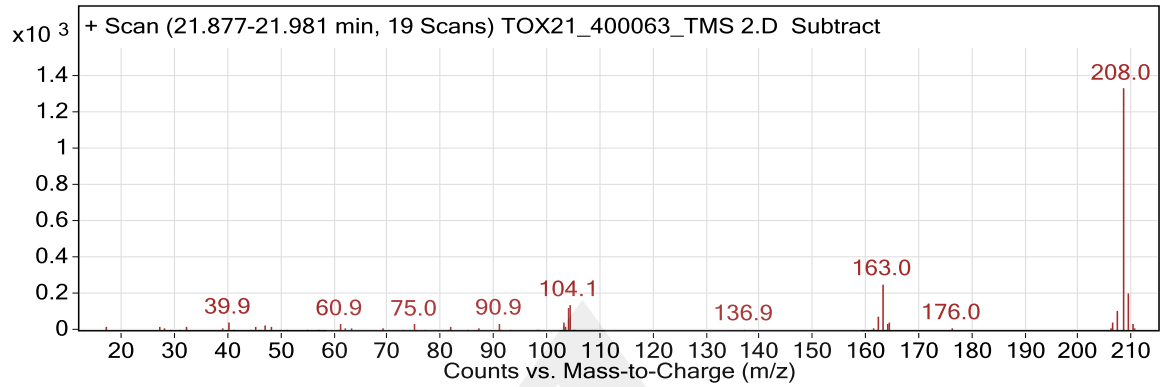

Spectrum Source
Peak (11) in "+ TIC Scan"

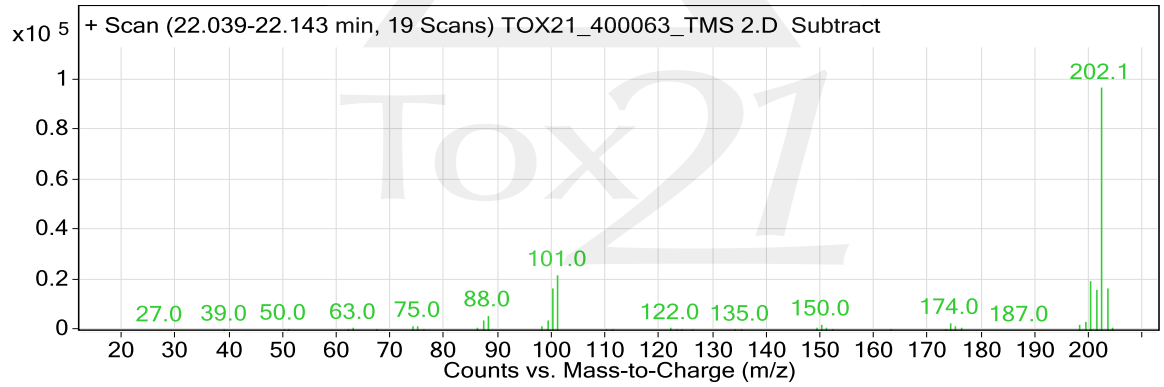

--- End Of Report ---

Qualitative Analysis Report

Data Filename	TOX21_400063_TMS 3.D	**Sample Name**	NCGC Tox21_400063 from B20 SP109729
Position	44	**Instrument Name**	5975C_MR
User Name	Long	**Acq Method**	C1_28-0_2_520_mt384_sndv.M

User Chromatograms

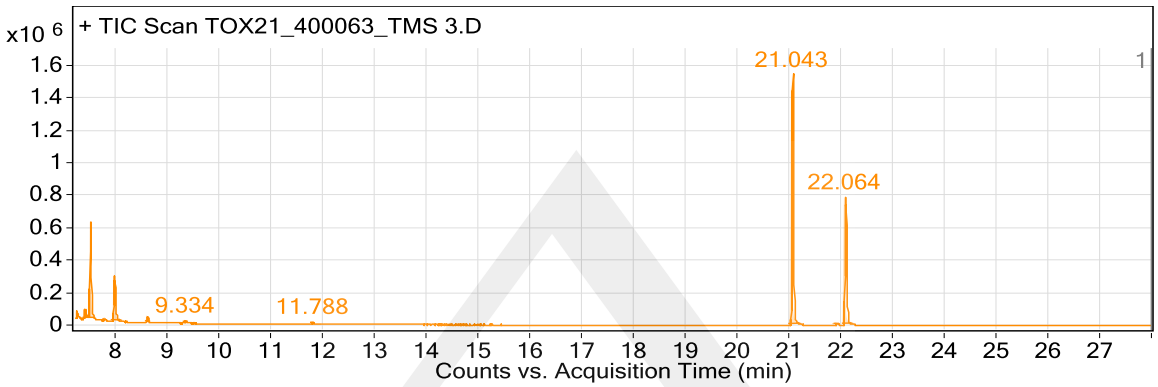

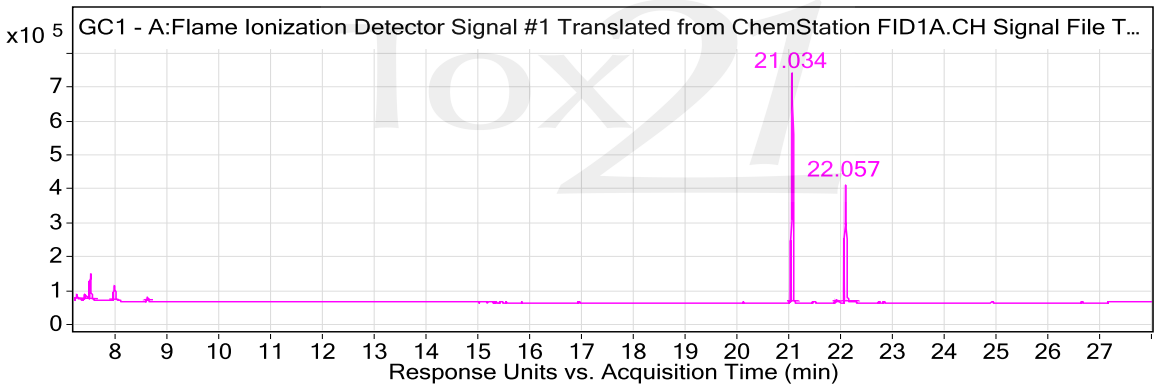

User Spectra

Spectrum Source
Peak (1) in "+ TIC Scan"

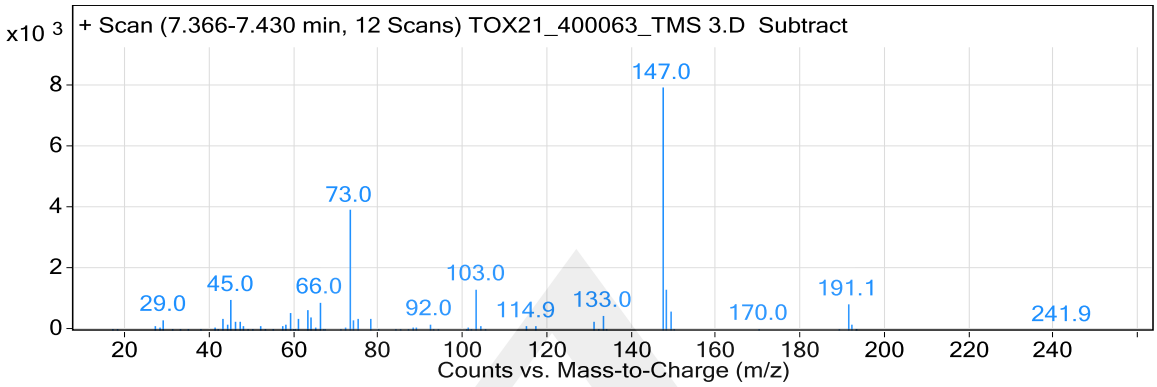

Spectrum Source
Peak (2) in "+ TIC Scan"

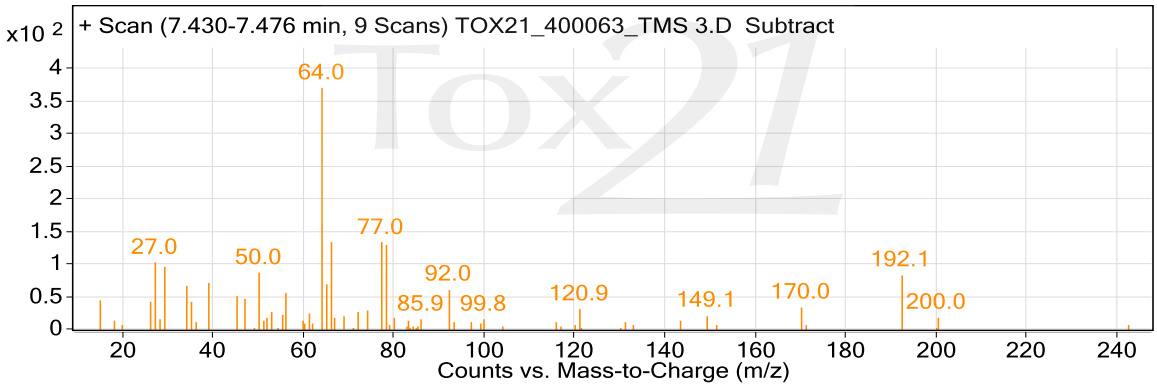

Spectrum Source
Peak (3) in "+ TIC Scan"

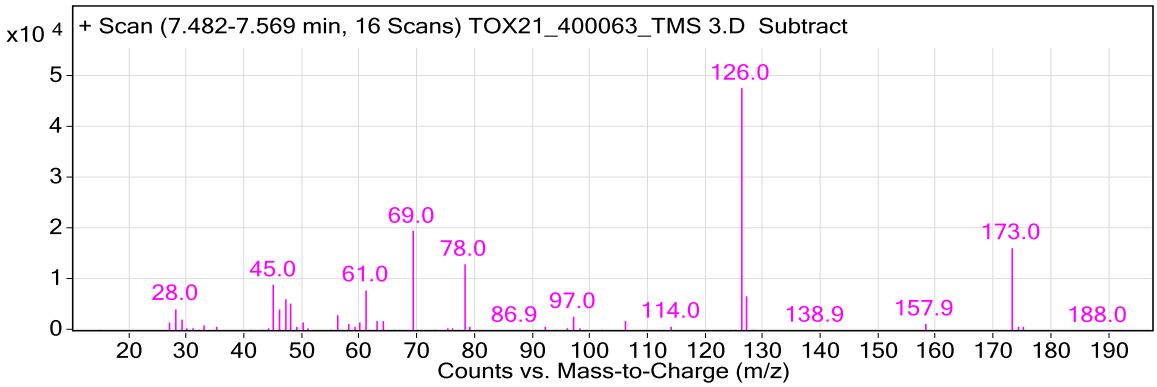

Spectrum Source
Peak (4) in "+ TIC Scan"

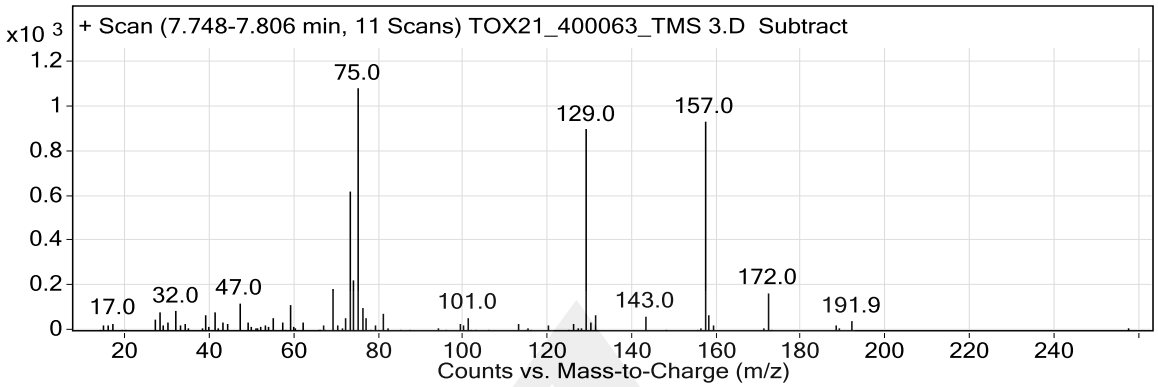

Spectrum Source
Peak (5) in "+ TIC Scan"

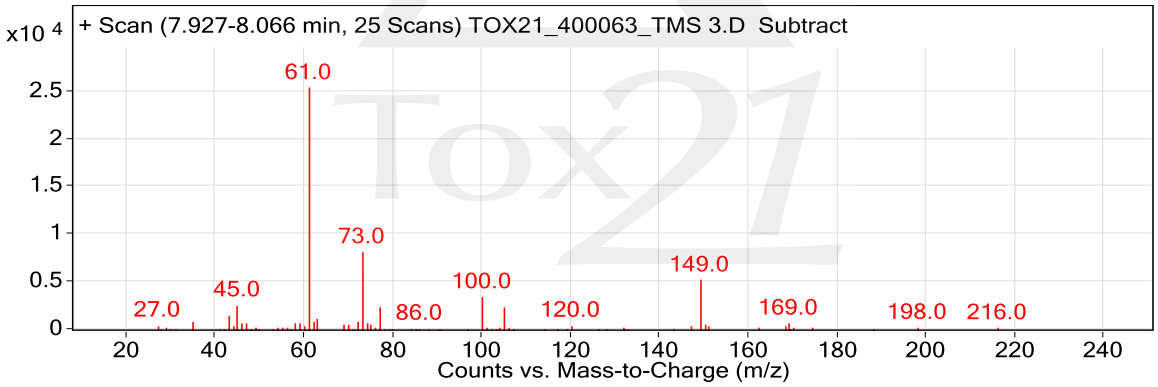

Spectrum Source
Peak (6) in "+ TIC Scan"

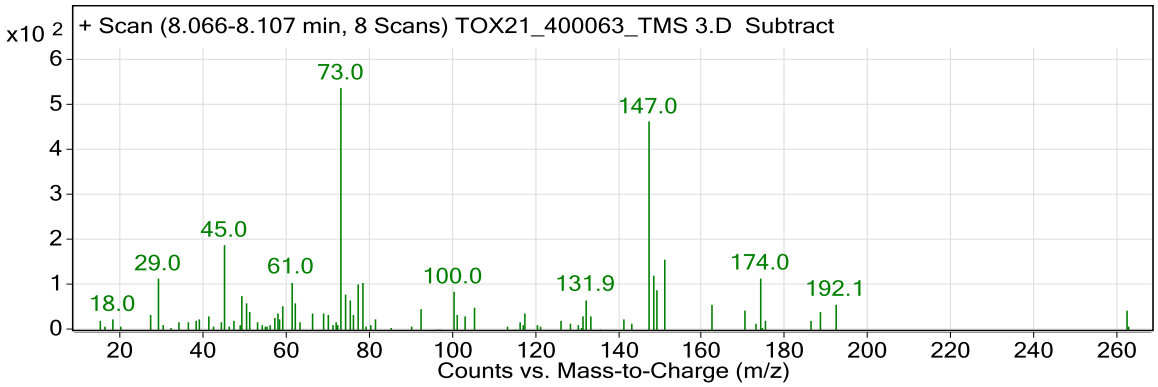

Spectrum Source
Peak (7) in "+ TIC Scan"

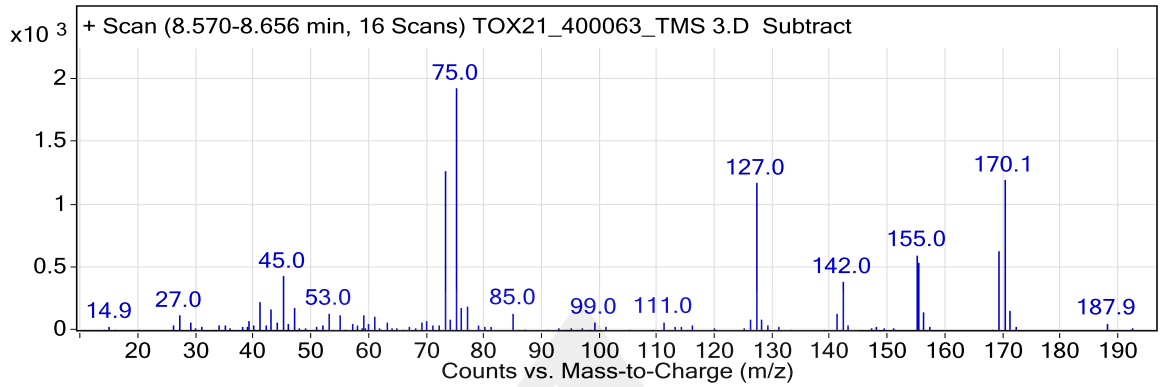

Spectrum Source
Peak (8) in "+ TIC Scan"

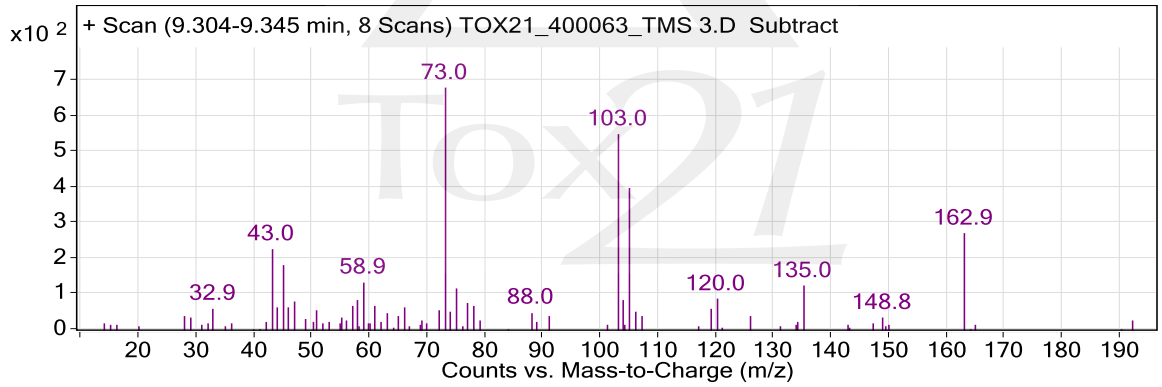

Spectrum Source
Peak (9) in "+ TIC Scan"

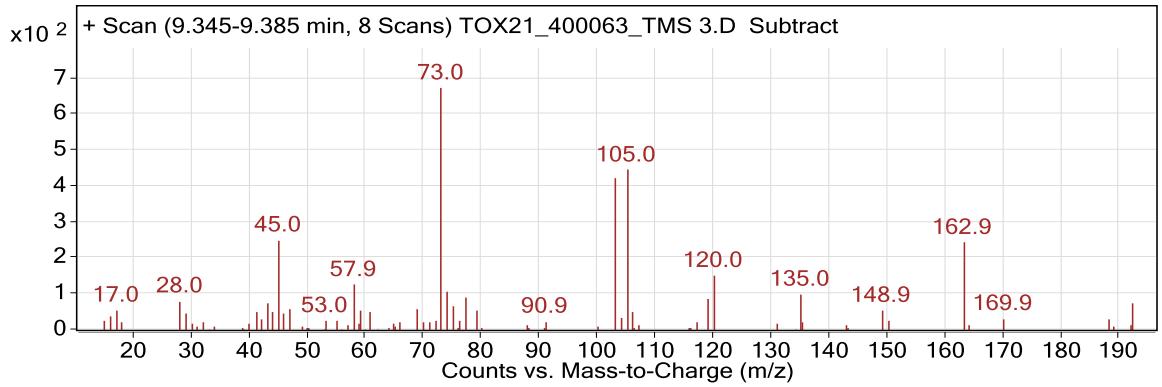

Spectrum Source
Peak (10) in "+ TIC Scan"

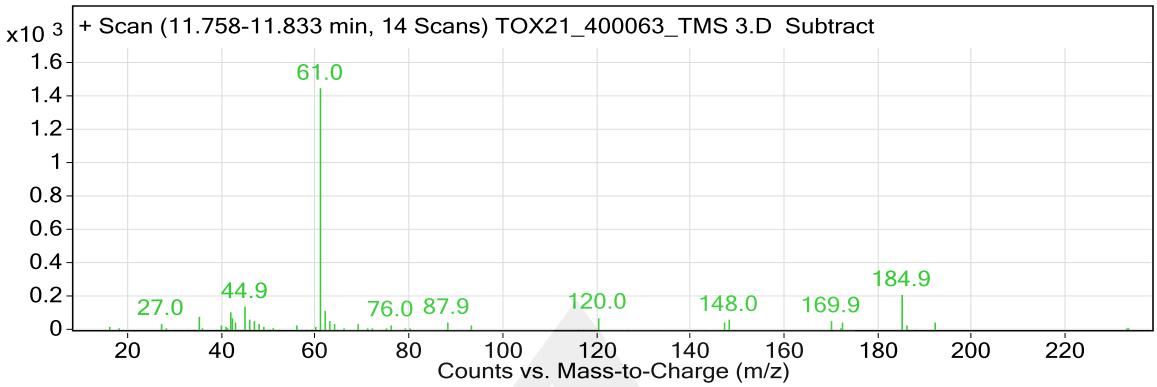

Spectrum Source
Peak (11) in "+ TIC Scan"

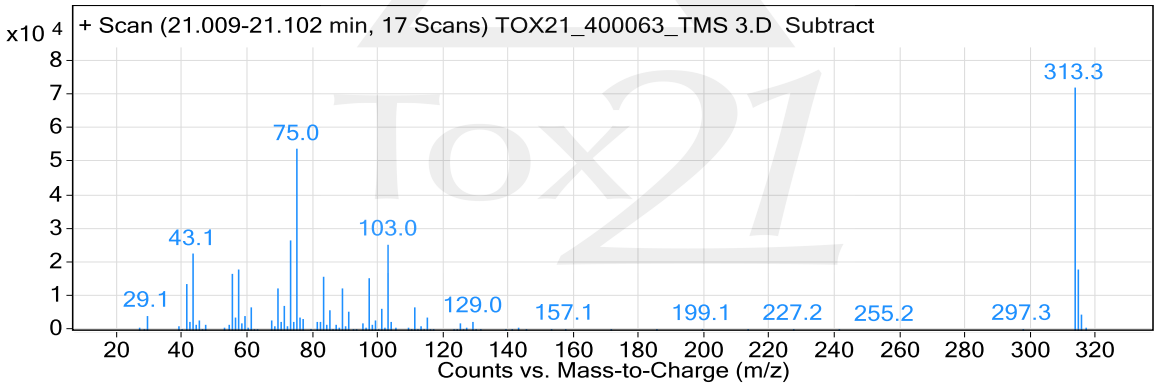

Spectrum Source
Peak (12) in "+ TIC Scan"

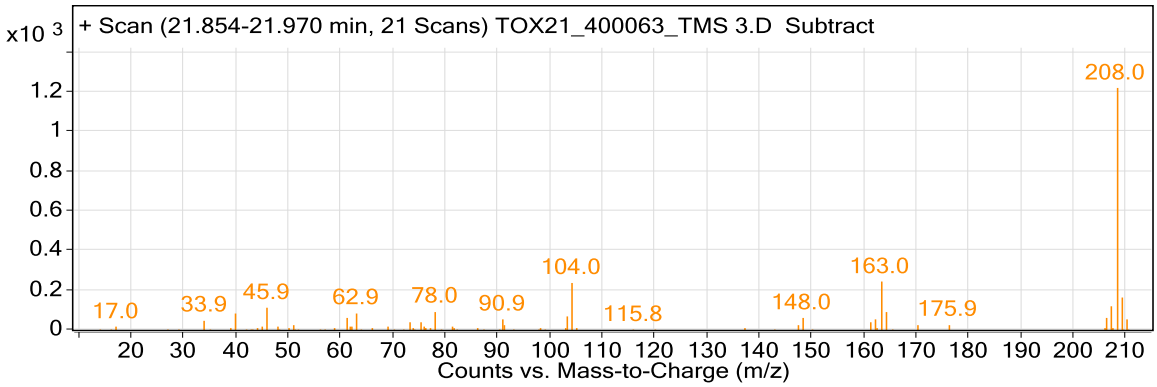

Spectrum Source
Peak (13) in "+ TIC Scan"

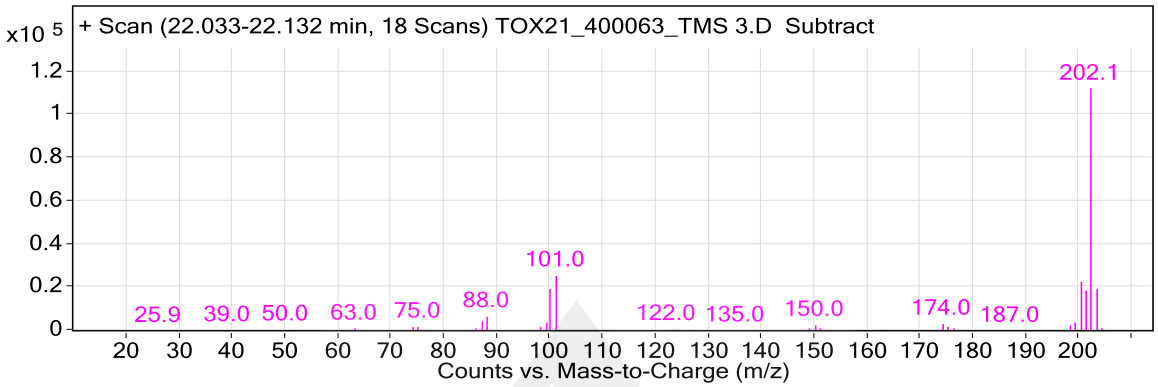

--- End Of Report ---

Qualitative Analysis Report

Data Filename	TOX21_400063_TMS 4.D	**Sample Name**	NCGC Tox21_400063 from M20 SP109738
Position	308	**Instrument Name**	5975C_MR
User Name	Long	**Acq Method**	C1_28-0_2_520_mt384_sndv.M

User Chromatograms

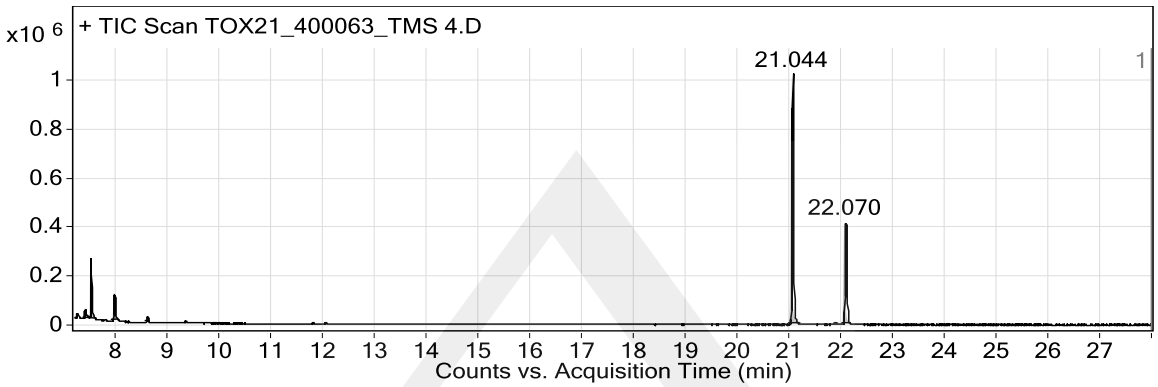

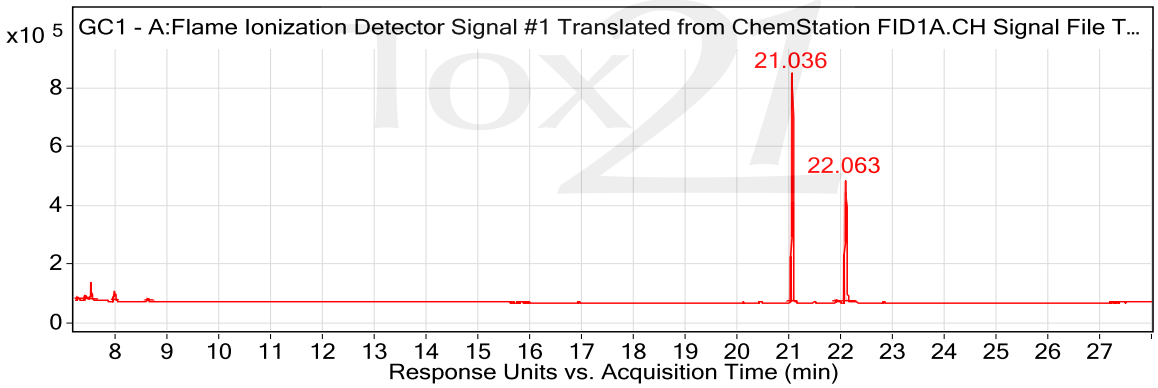

User Spectra

Spectrum Source
Peak (1) in "+ TIC Scan"

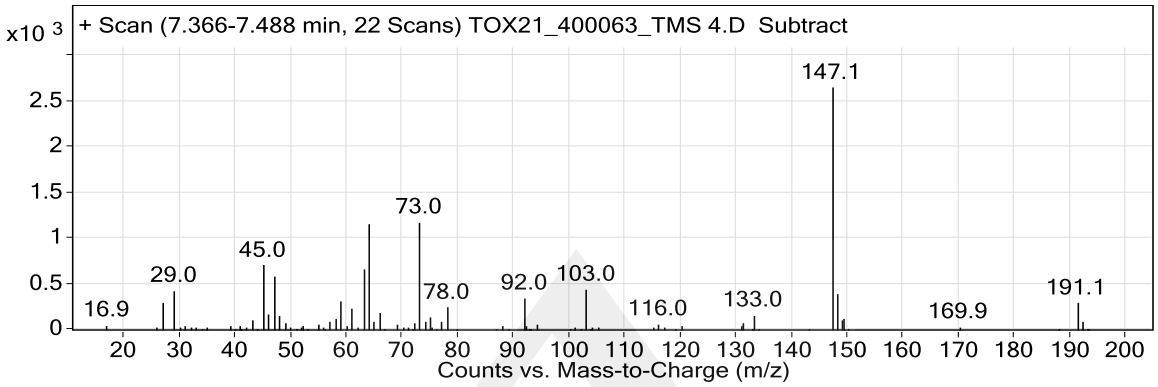

Spectrum Source
Peak (2) in "+ TIC Scan"

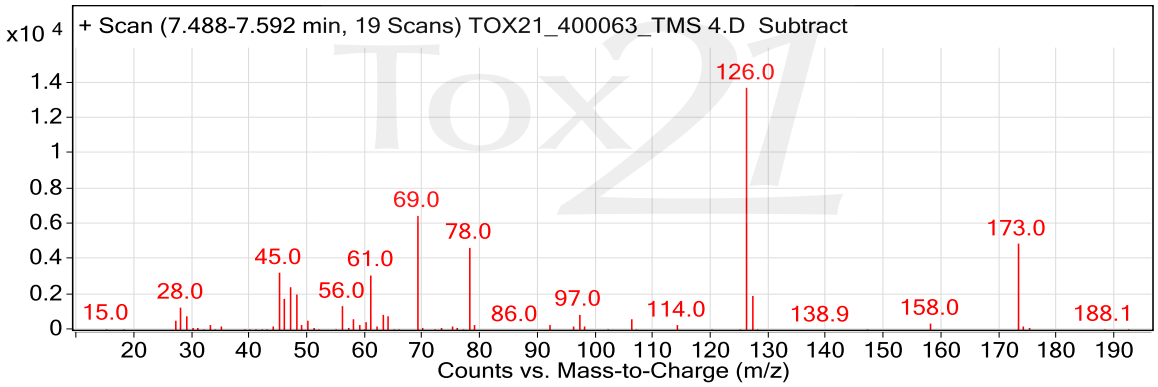

Spectrum Source
Peak (3) in "+ TIC Scan"

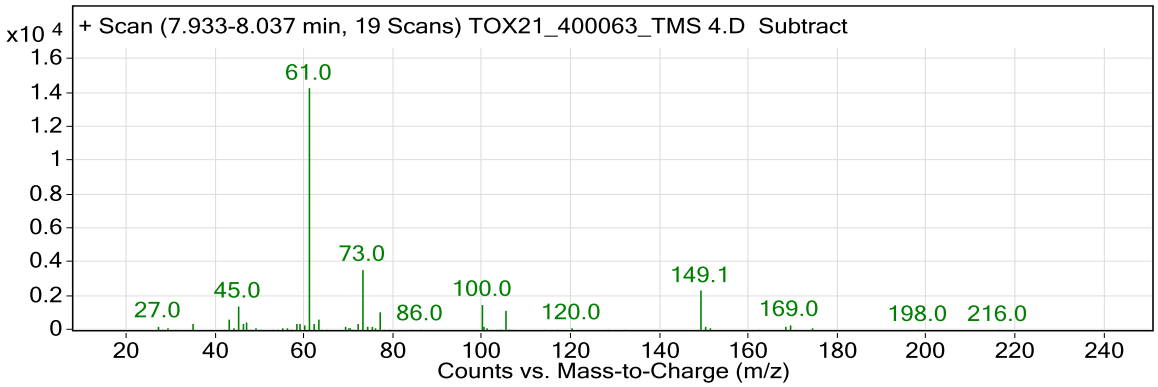

Spectrum Source
Peak (4) in "+ TIC Scan"

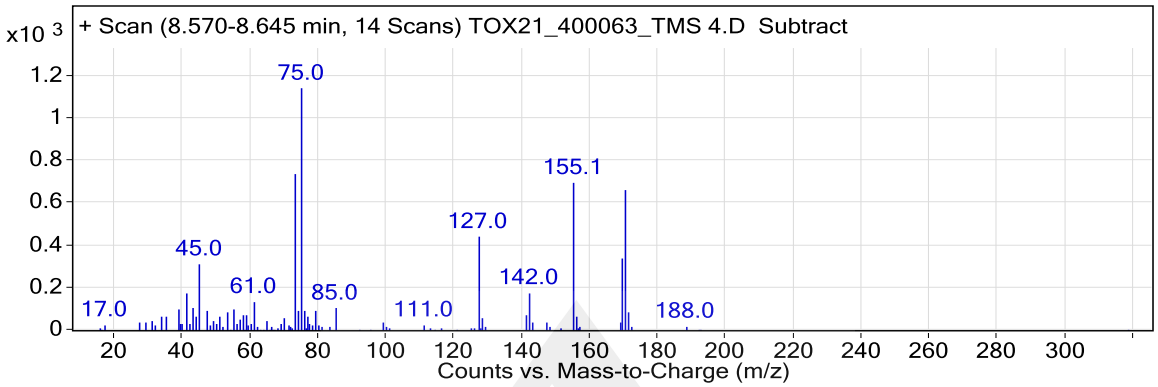

Spectrum Source
Peak (5) in "+ TIC Scan"

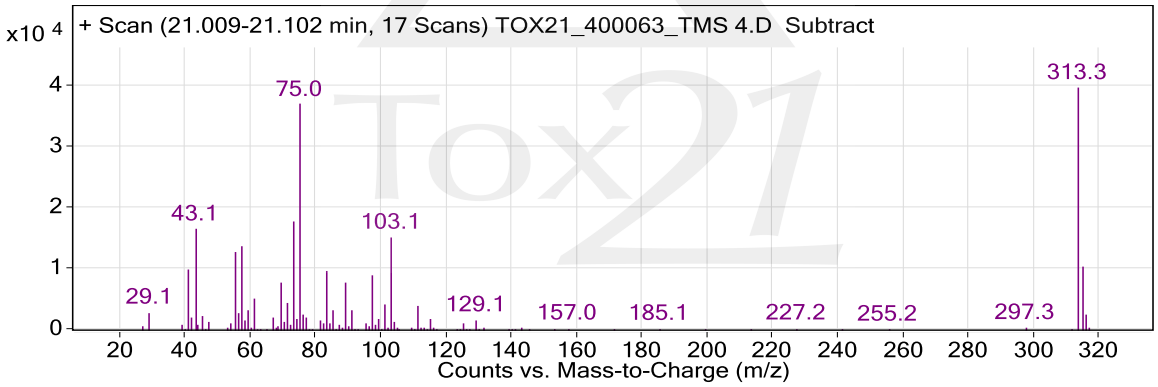

Spectrum Source
Peak (6) in "+ TIC Scan"

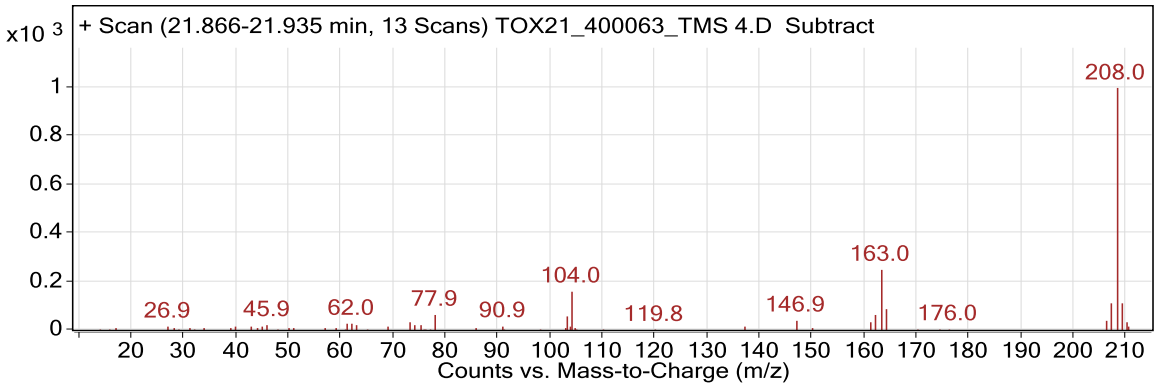

Spectrum Source
Peak (7) in "+ TIC Scan"

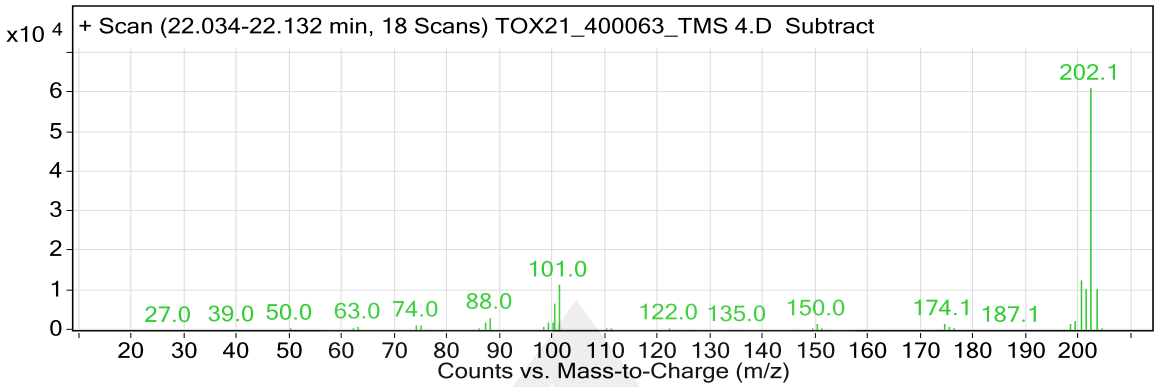

--- End Of Report ---

Qualitative Analysis Report

Data Filename	TOX21_400063_TMS 5.D	**Sample Name**	NCGC Tox21_400063 from M20 SP109778
Position	308	**Instrument Name**	5975C_MR
User Name	Long	**Acq Method**	C1_28-0_2_520_mt384_sndv.M

User Chromatograms

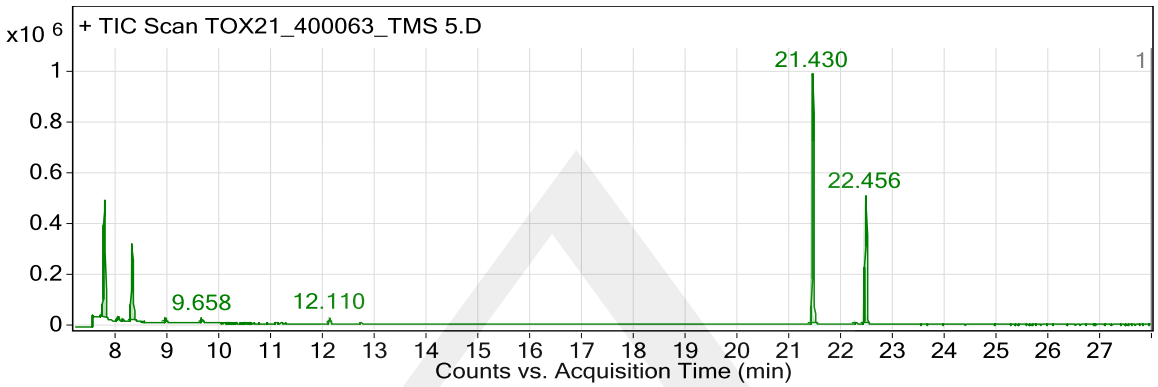

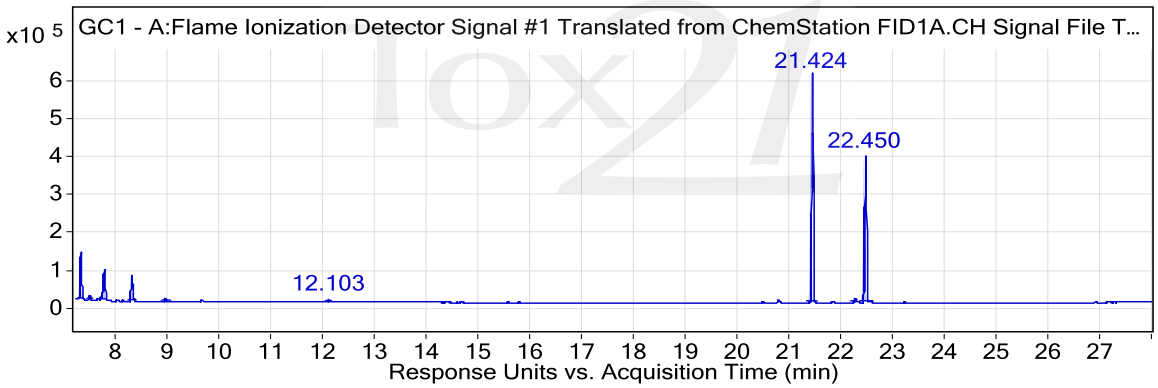

User Spectra

Spectrum Source
Peak (1) in "+ TIC Scan"

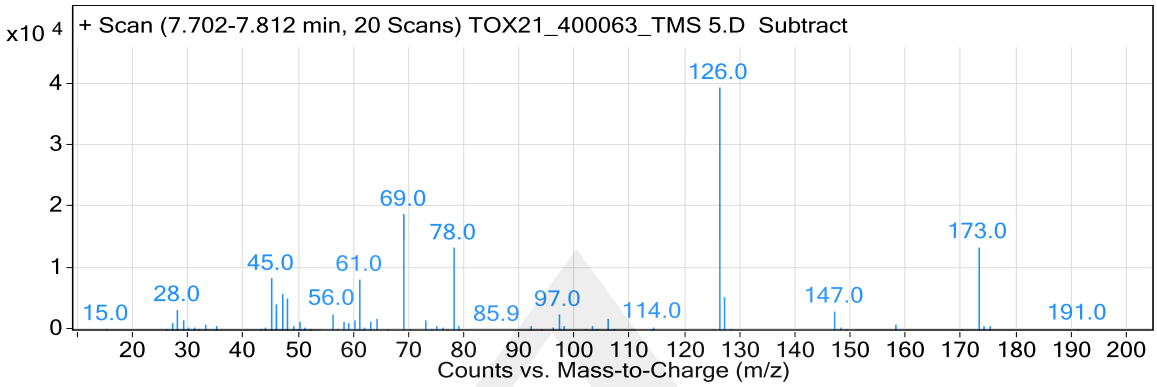

Spectrum Source
Peak (2) in "+ TIC Scan"

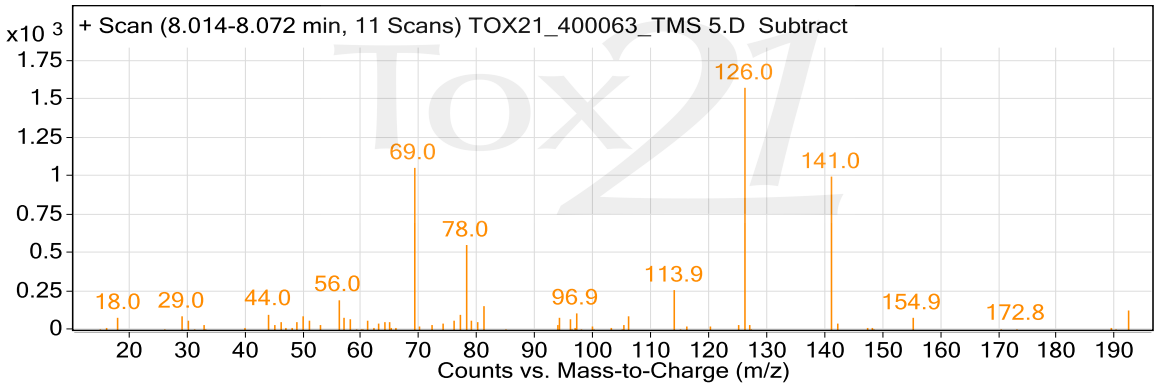

Spectrum Source
Peak (3) in "+ TIC Scan"

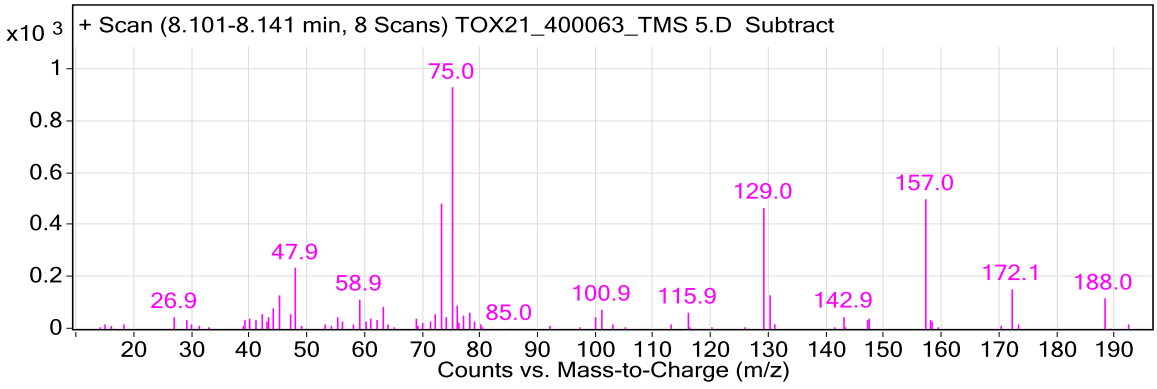

Spectrum Source
Peak (4) in "+ TIC Scan"

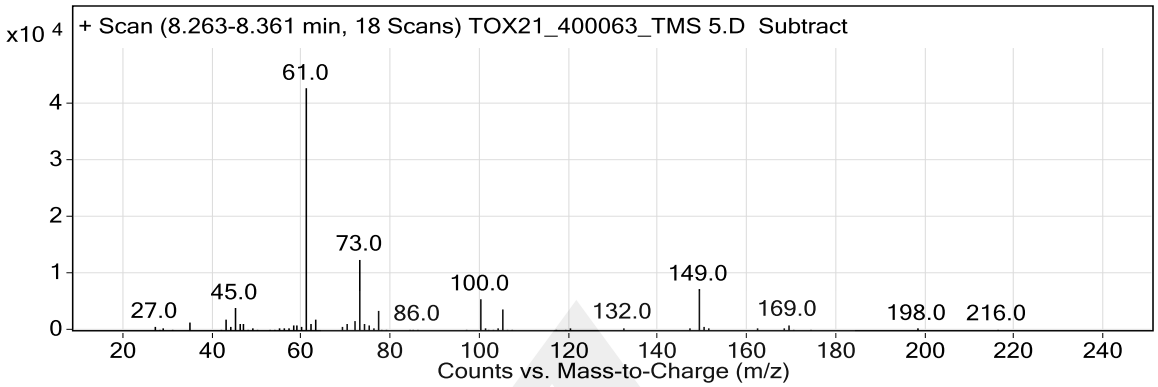

Spectrum Source
Peak (5) in "+ TIC Scan"

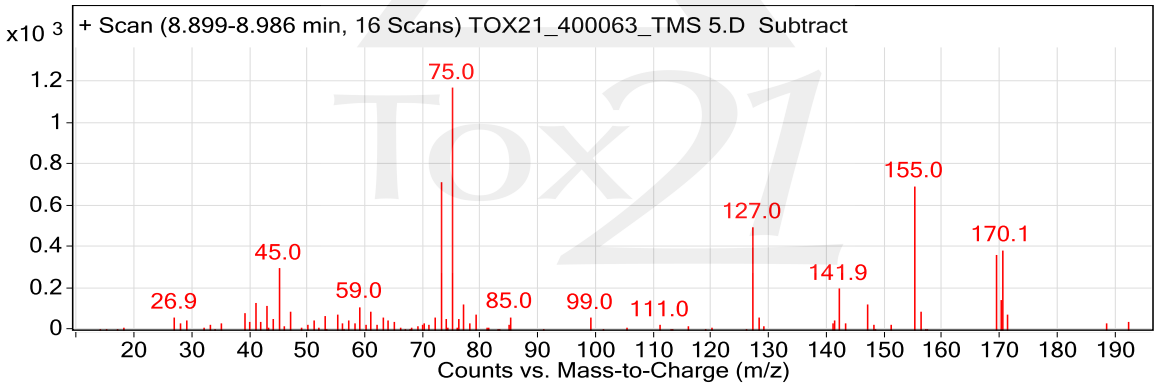

Spectrum Source
Peak (6) in "+ TIC Scan"

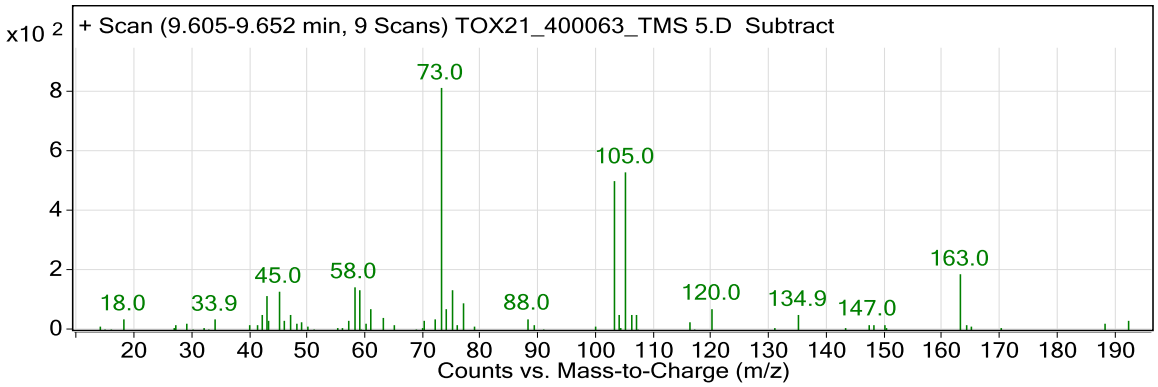

Spectrum Source
Peak (7) in "+ TIC Scan"

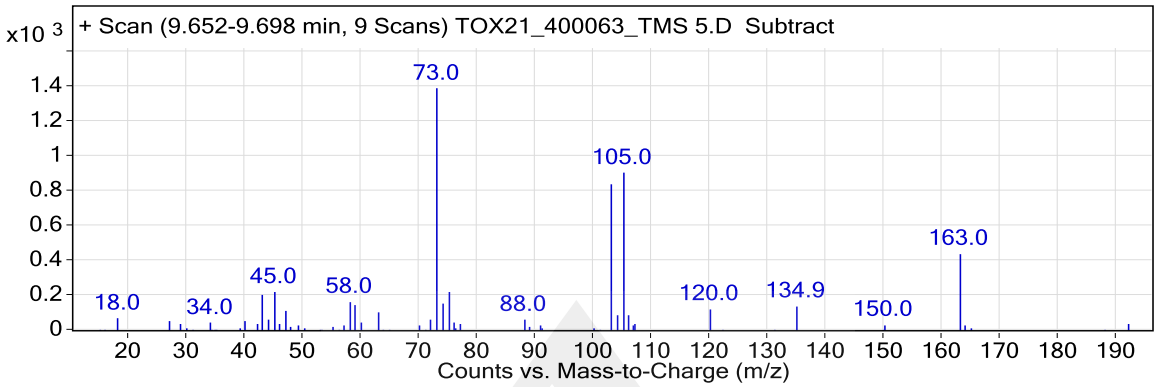

Spectrum Source
Peak (8) in "+ TIC Scan"

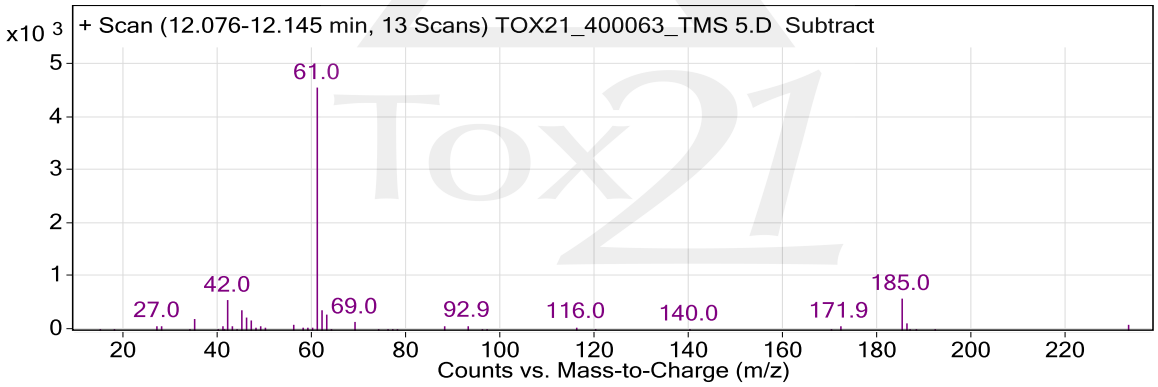

Spectrum Source
Peak (9) in "+ TIC Scan"

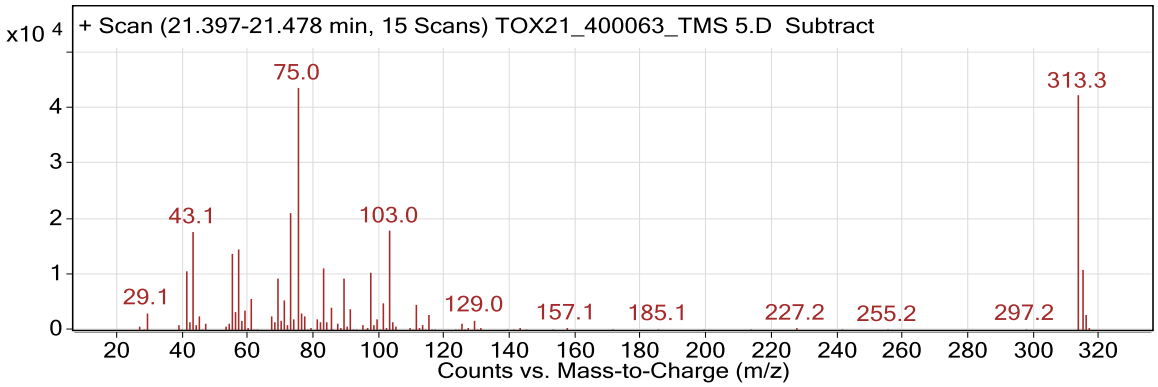

Spectrum Source
Peak (10) in "+ TIC Scan"

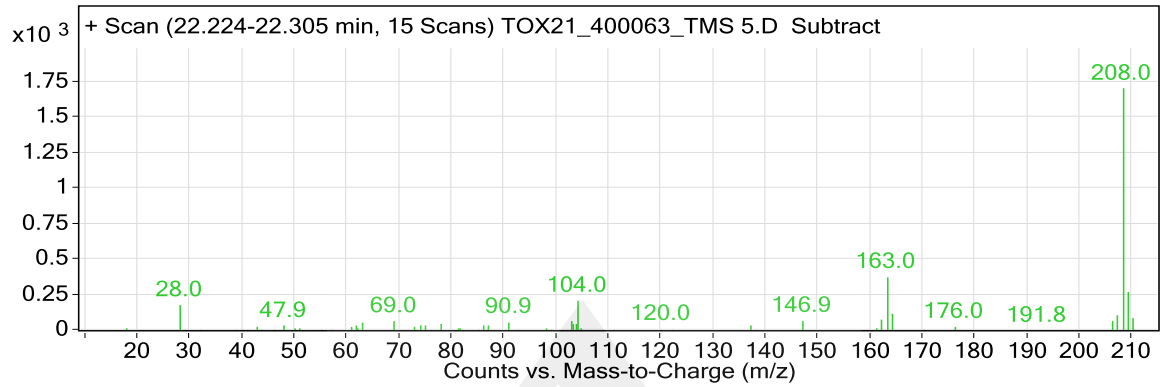

Spectrum Source
Peak (11) in "+ TIC Scan"

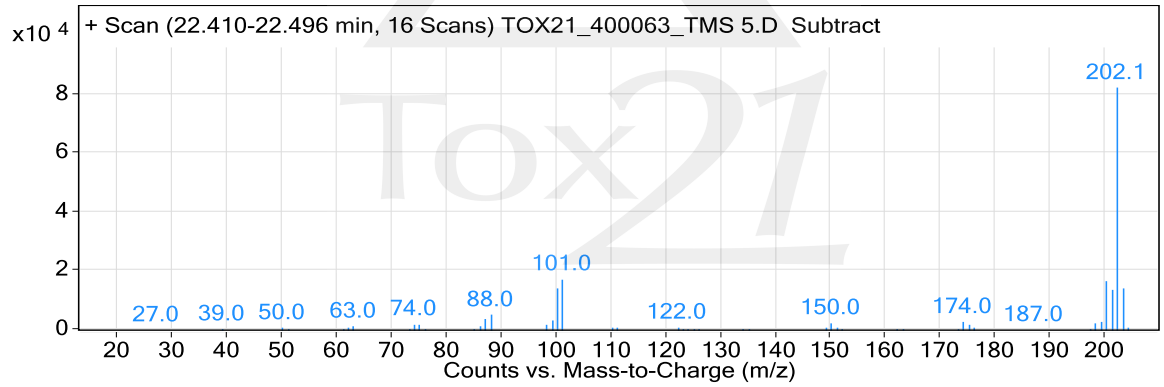

--- End Of Report ---

Qualitative Analysis Report

Data Filename	TOX21_400063_TMS 6.D	**Sample Name**	NCGC Tox21_400063 from E13 SP109798
Position	109	**Instrument Name**	5975C_MR
User Name	Long	**Acq Method**	C1_28-0_2_520_mt384_sndv.M

User Chromatograms

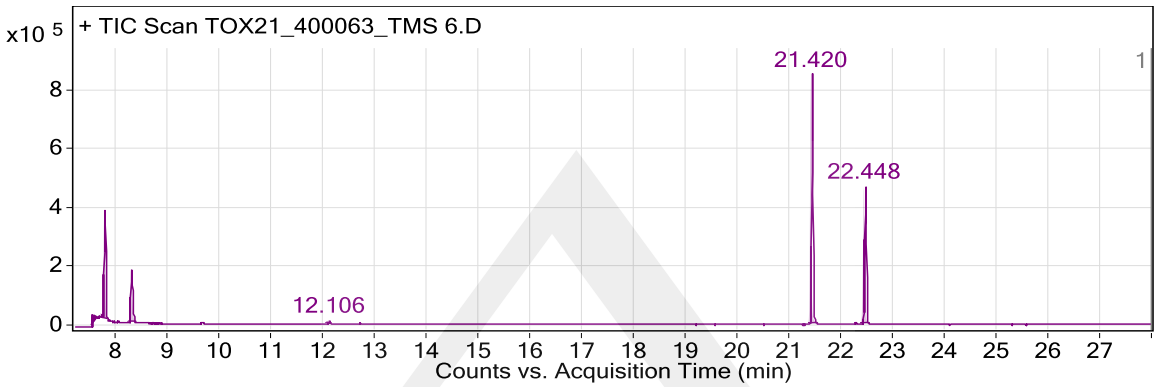

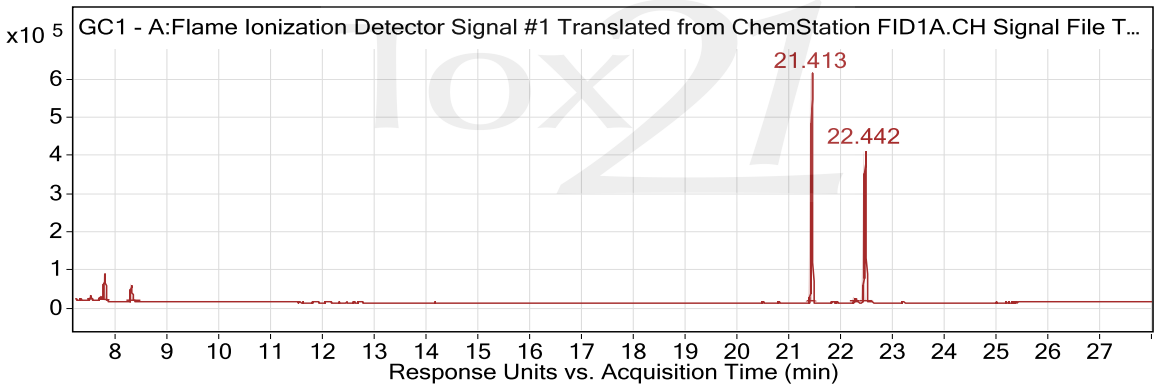

User Spectra

Spectrum Source
Peak (1) in "+ TIC Scan"

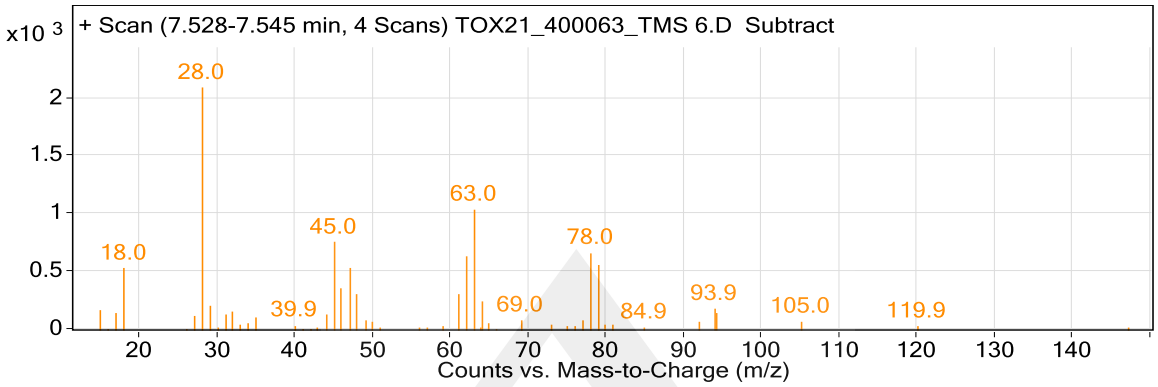

Spectrum Source
Peak (2) in "+ TIC Scan"

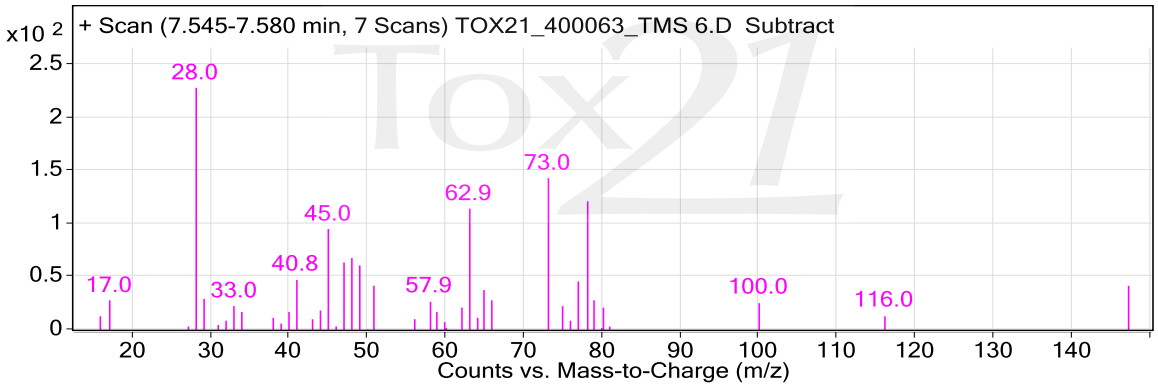

Spectrum Source
Peak (3) in "+ TIC Scan"

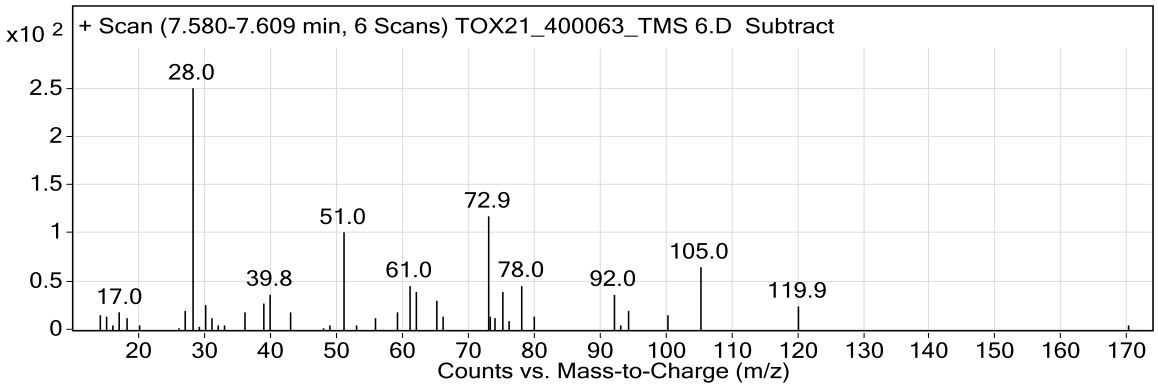

Spectrum Source
Peak (4) in "+ TIC Scan"

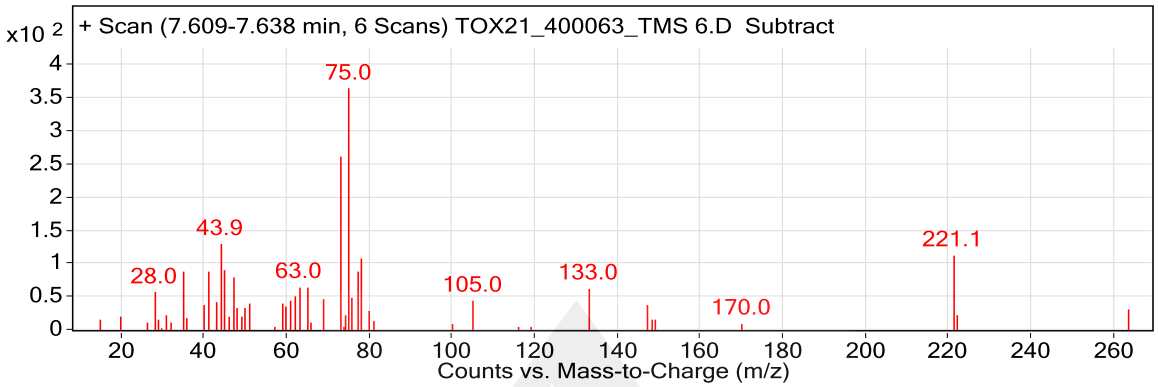

Spectrum Source
Peak (5) in "+ TIC Scan"

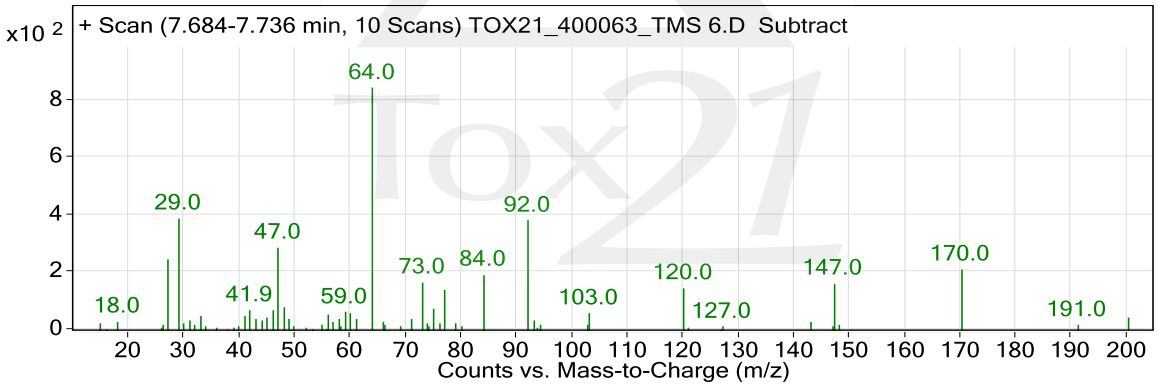

Spectrum Source
Peak (6) in "+ TIC Scan"

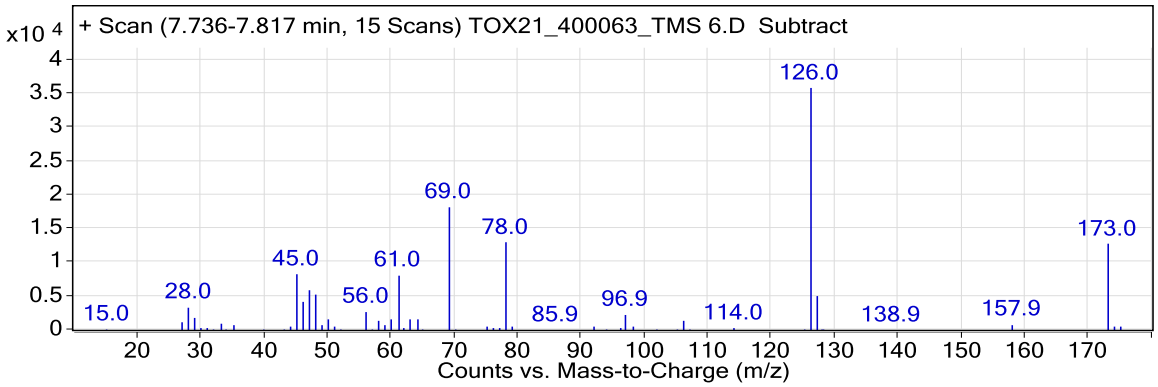

Spectrum Source
Peak (7) in "+ TIC Scan"

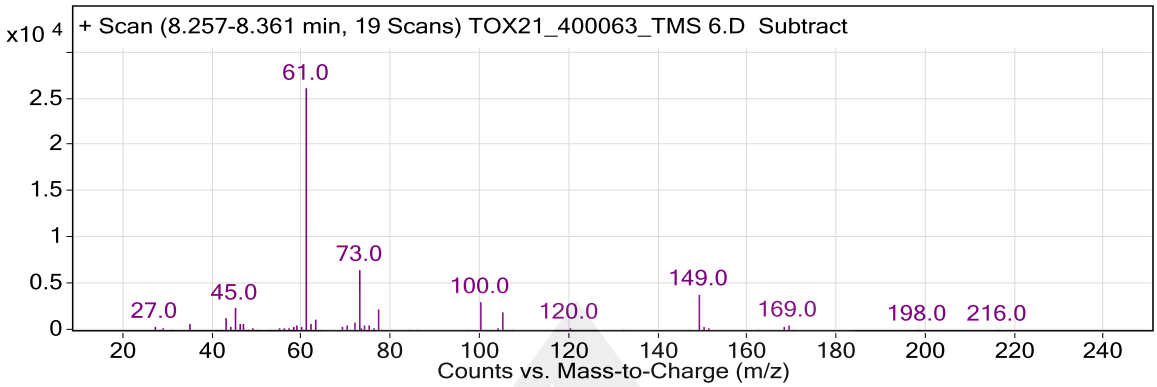

Spectrum Source
Peak (8) in "+ TIC Scan"

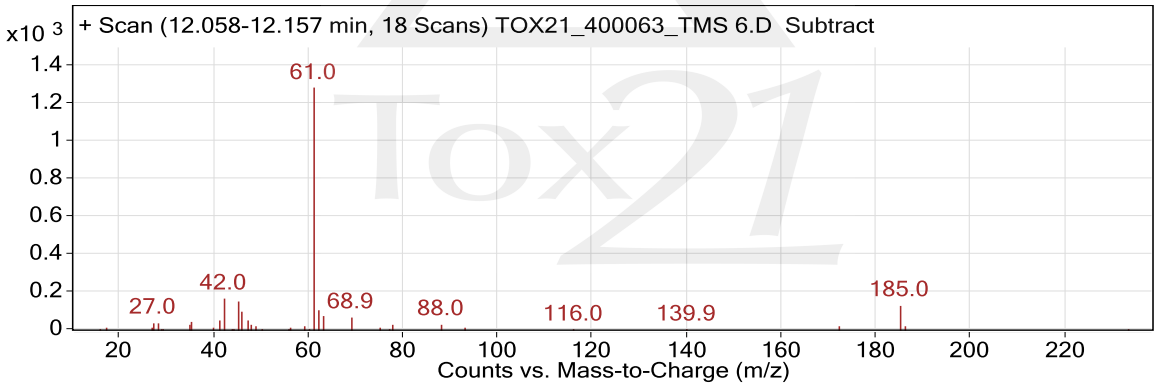

Spectrum Source
Peak (9) in "+ TIC Scan"

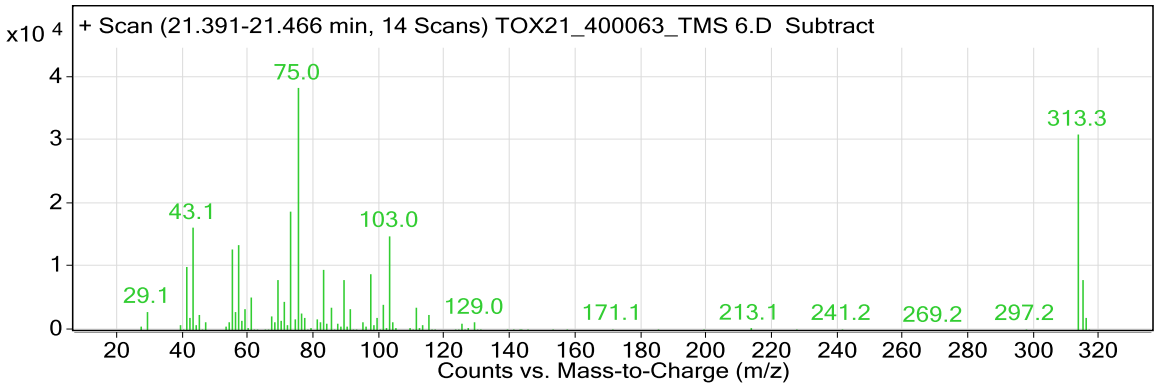

Spectrum Source
Peak (10) in "+ TIC Scan"

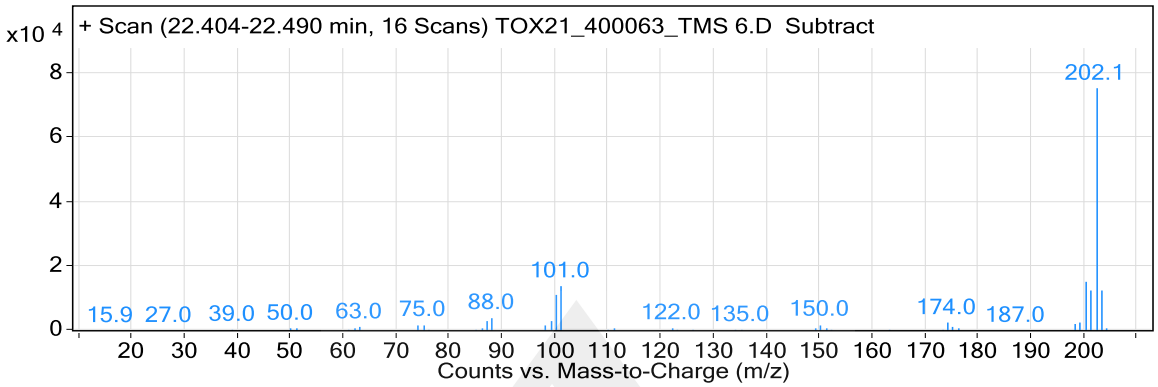

--- End Of Report ---